

PHILIPS BV Pulsera
H Unimed Florianópolis


Patient
SAMUEL BUZZI RAMOS
2511019
19-04-2007 M
Examination

Orthopaedics
19-03-2022

Examination dose
0.351 mGy

2 (10:55)
1

Image is being stored to USB memory stick, wait for completion

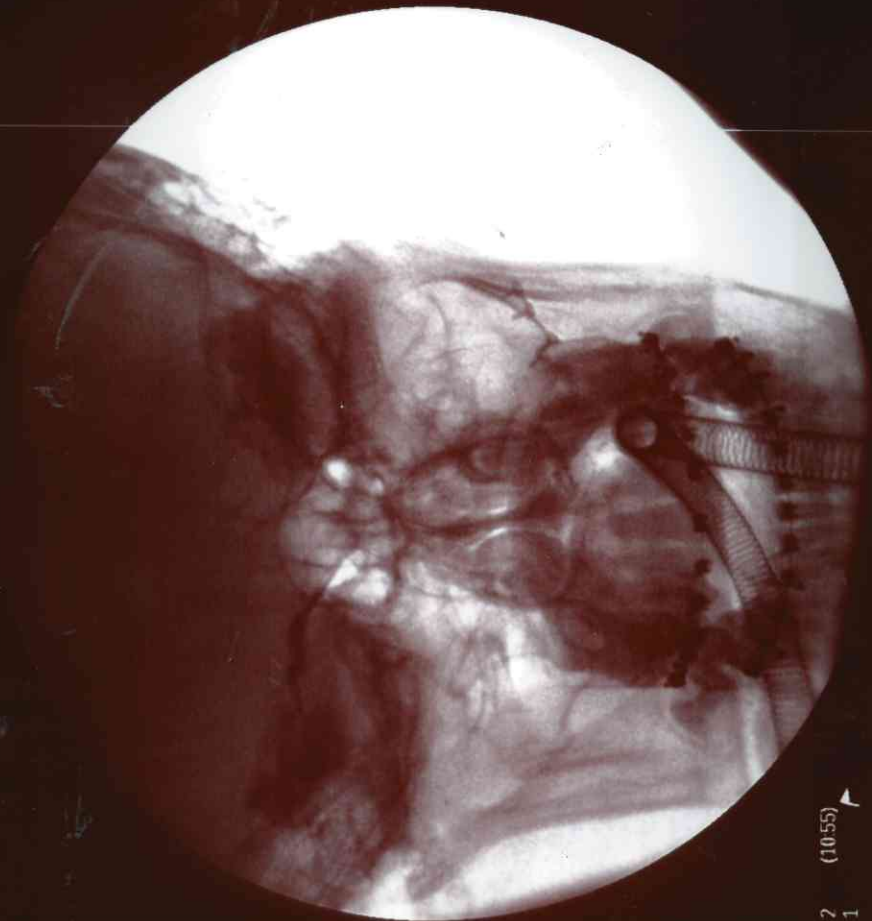

PHILIPS BV Pulsera
H. Unimed Florianópolis

Patient

SAMUEL BUZZI RAMOS

2511019

19-04-2007 M

Examination

Orthopaedics

19-03-2022

Examination dose
0.351 mGy

3 (10:58)
1

Image is being stored to USB memory stick, wait for completion



SAMUEL BUZZI RAMOS

Instituto Adventista

Atend: 2511019 205 APTO

Dt Nas: 19/04/07



CAIXA REDONDA 200 ML

Ciclo: 7409

Esterilização: 18/03/2022 07:00:00

Validade: 06/07/2022 06:23:29

Método: VAPOR SATURADO SOB PRESSÃO (121 C)

Responsável: michela.vicente



923145

CAIXA BUCOMAXILO TRAUMA

Ciclo: 7510

Esterilização: 11/03/2022 05:28:04

Validade: 09/07/2022 05:20:37

Método: VAPOR SATURADO SOB PRESSÃO (134 C)

Responsável: anemachado



918766

CAIXA SEPTOPLASTIA

Ciclo: 7393

Esterilização: 15/03/2022 20:13:54

Validade: 13/07/2022 19:09:34

Método: VAPOR SATURADO SOB PRESSÃO (134 C)

Responsável: michela.vicente



921657

MATERIAL ORTOFACE

Ciclo: 7533

Esterilização: 18/03/2022 19:02:23

Validade: 16/07/2022 20:32:51

Método: VAPOR SATURADO SOB PRESSÃO (121 C)

Responsável: adriane.feria



923301

MATERIAL DR. EDUARDO MEUREP

Ciclo: 5314

Esterilização: 11/03/2022 04:53:58

Validade: 09/07/2022 05:15:48

Método: VAPOR DE PEROXIDO DE HIDROGENIO (45 C)

Responsável: anemachado



918738

F10 MONONYLON 2-0 (1215T) - ETHICON
L: AR5636
V: 30/11/2026 C: 63000
00005099870

F10 BIOSYN 5-0 15MS
6872 COVIDIEN
L: D9G1551FY
V: 30/06/2024 C: 81118
00005060737

Monofilament Glycomer™ 631
Monofilament de Glycomer™ 631
Glycomer™ 631, monofil
Glycomer™ 631 monofilamento
Glycomer™ 631 monofilamento
Synthetic Absorbable Suture
Suture synthétique résorbable
Resorbierbare Fäden, synthetisch
Filo di sutura sintetica, assorbibile
Sutura sintética absorbível
Biosyn™ sutures are USP/EP
except for diameter
Syneture™

STERILE EO

CE 0123

Single use Caution, consult
accompanying documents

(01)10984521033139
(17)240630
(10)D9G1551FY

LOT D9G1551FY
Use by 2024-06-30
REF SM5687

